


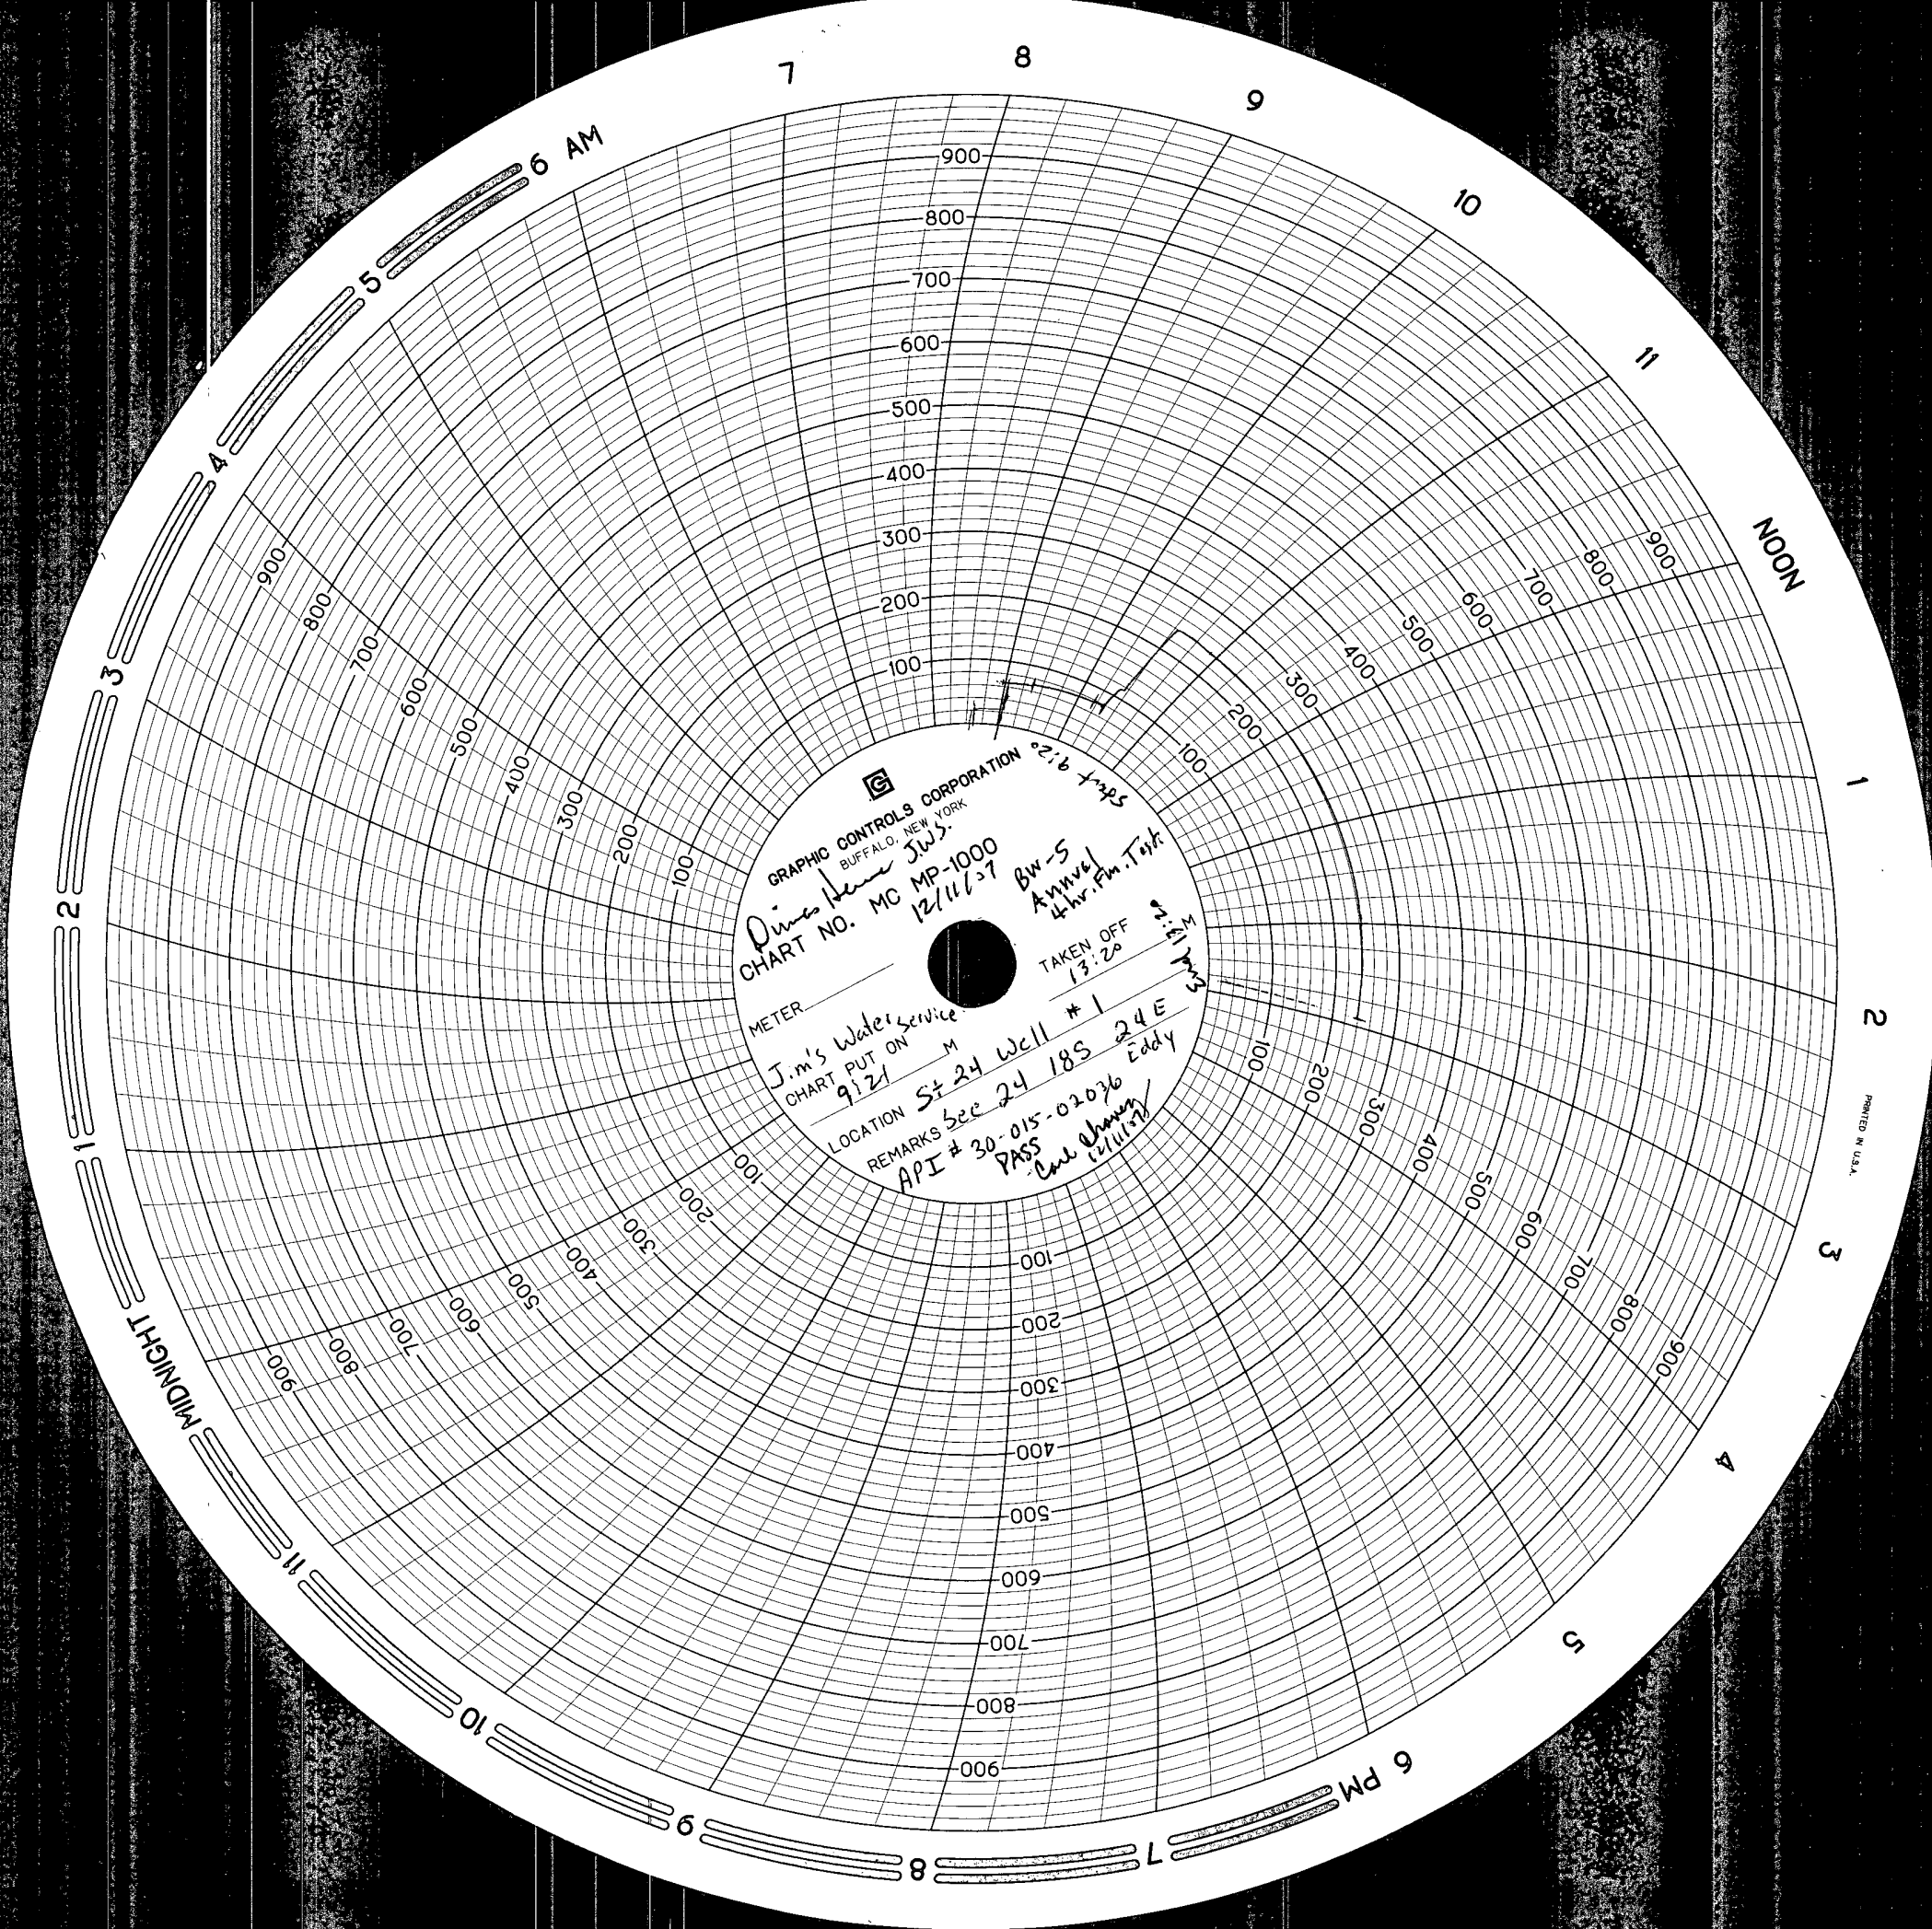

Wildcat Measurement

Calibration Certificate

Pressure Recorder

Serial Number: 265-WC060224

Pressure Range 1000# p.s.i. accuracy +/- 0.2% % Full Scale _____ p.s.i. _____

Increasing Pressure			Decreasing Pressure		
Applied Pressure	Indicated Pressure	Difference	Applied Pressure	Indicated Pressure	Difference
0.0#	0.0#	0.0#	800.0#	800.0#	0.0#
100.0#	100.0#	0.0#	600.0#	600.0#	0.0#
300.0#	300.0#	0.0#	400.0#	400.0#	0.0#
500.0#	500.0#	0.0#	200.0#	200.0#	0.0#
700.0#	700.0#	0.0#	0.0#	0.0#	0.0#
1000.0#	1000.0#	0.0#			

Calibrated By: Crystal Gauge Deadweight _____

This Is To Certify That This Recorder Has Been Inspected And Tested.

Remarks _____

Date Of Calibration 12-07-2007 Inspector 