


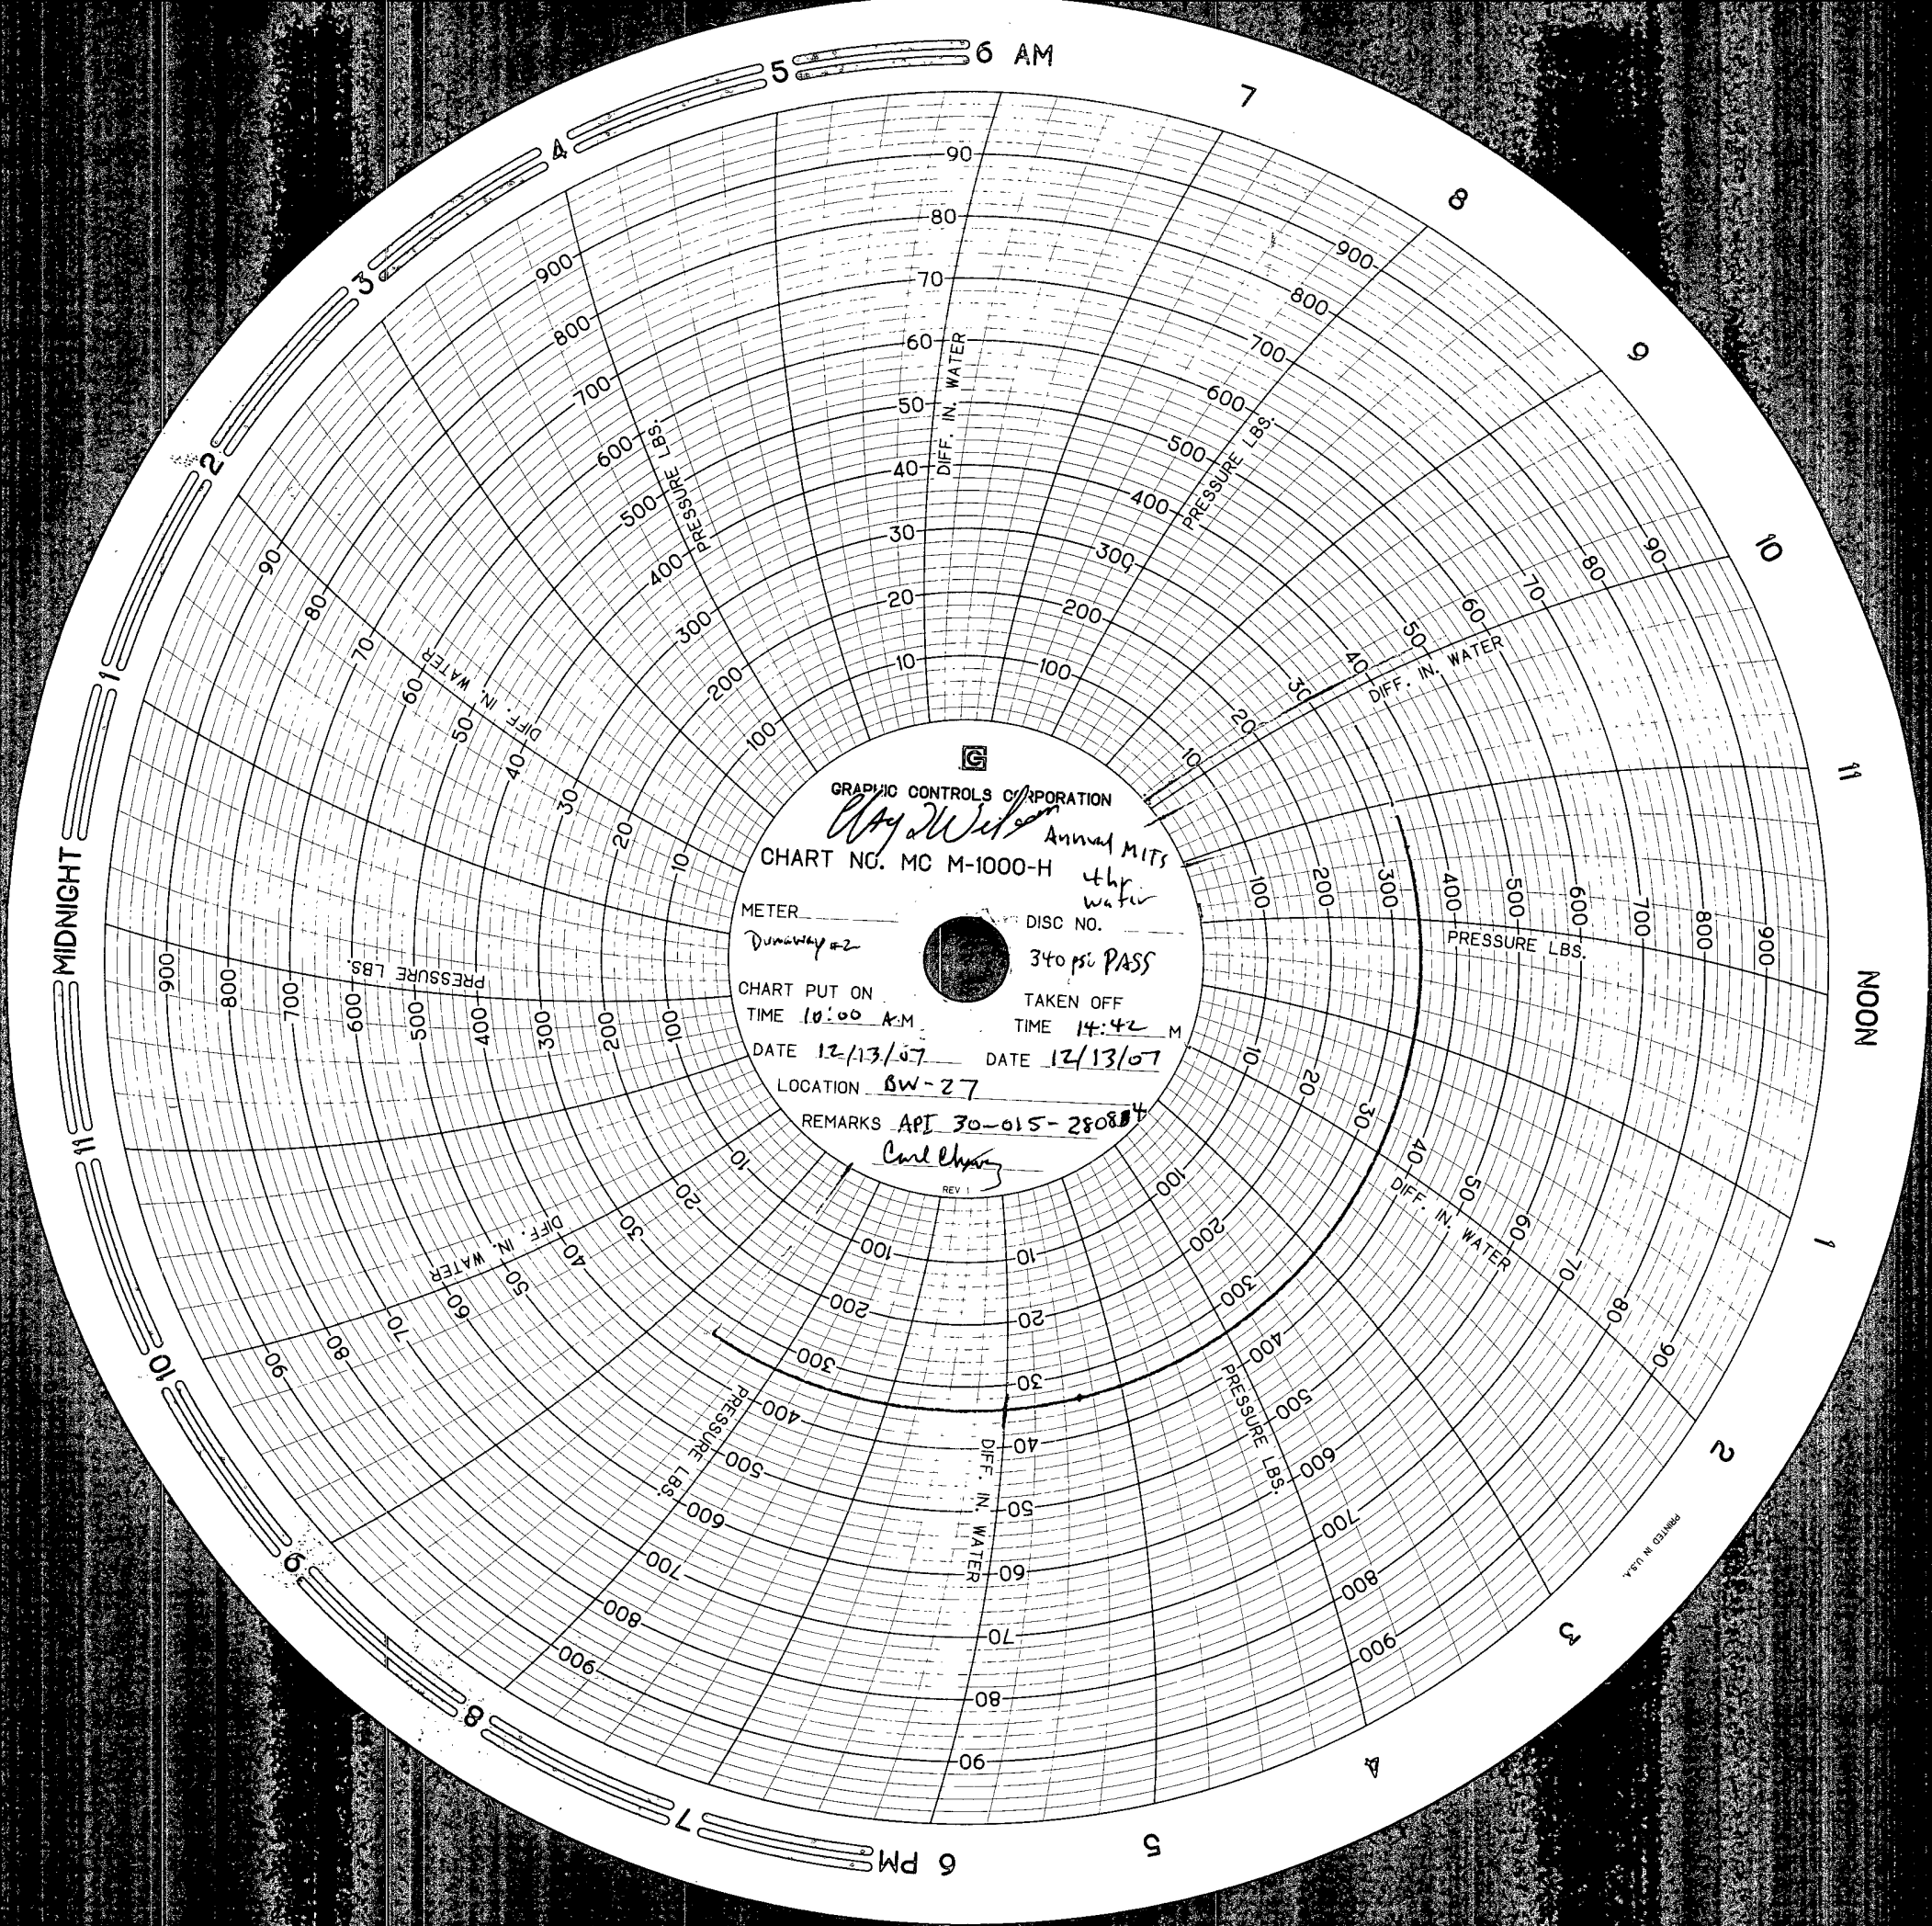

American Valve & Meter, Inc.

1113 W. BROADWAY

P.O. BOX 166

HOBBS, NM 88240

TO: Mesquite SWP

DATE: 12-12-07

This is to certify that:

I, Austin, Technician for American Valve & Meter,

Inc., has checked the calibration of the following instrument.

1000" Pressure Recorder Serial No: 265 45 44

at these points.

Pressure 1000"

Temperature _____

<u>Test</u>	<u>Found</u>	<u>Left</u>	<u>Test</u>	<u>Found</u>	<u>Left</u>
<u>0</u>	<u>—</u>	<u>0</u>	<u>—</u>	<u>—</u>	<u>—</u>
<u>500</u>	<u>✓</u>	<u>500</u>	<u>—</u>	<u>—</u>	<u>—</u>
<u>1000</u>	<u>✓</u>	<u>1000</u>	<u>—</u>	<u>—</u>	<u>—</u>
<u>800</u>	<u>✓</u>	<u>800</u>	<u>—</u>	<u>—</u>	<u>—</u>
<u>200</u>	<u>✓</u>	<u>200</u>	<u>—</u>	<u>—</u>	<u>—</u>
<u>0</u>	<u>✓</u>	<u>0</u>	<u>—</u>	<u>—</u>	<u>—</u>

Remarks: _____

Signature Austin