


**DEC 14, 2020- TOE PREP AND PRESSURE TEST 5.5" PRODUCTION
CASING TO 4400 PSI-HELD CHART ATTACHED WITH CALIBRATION.**

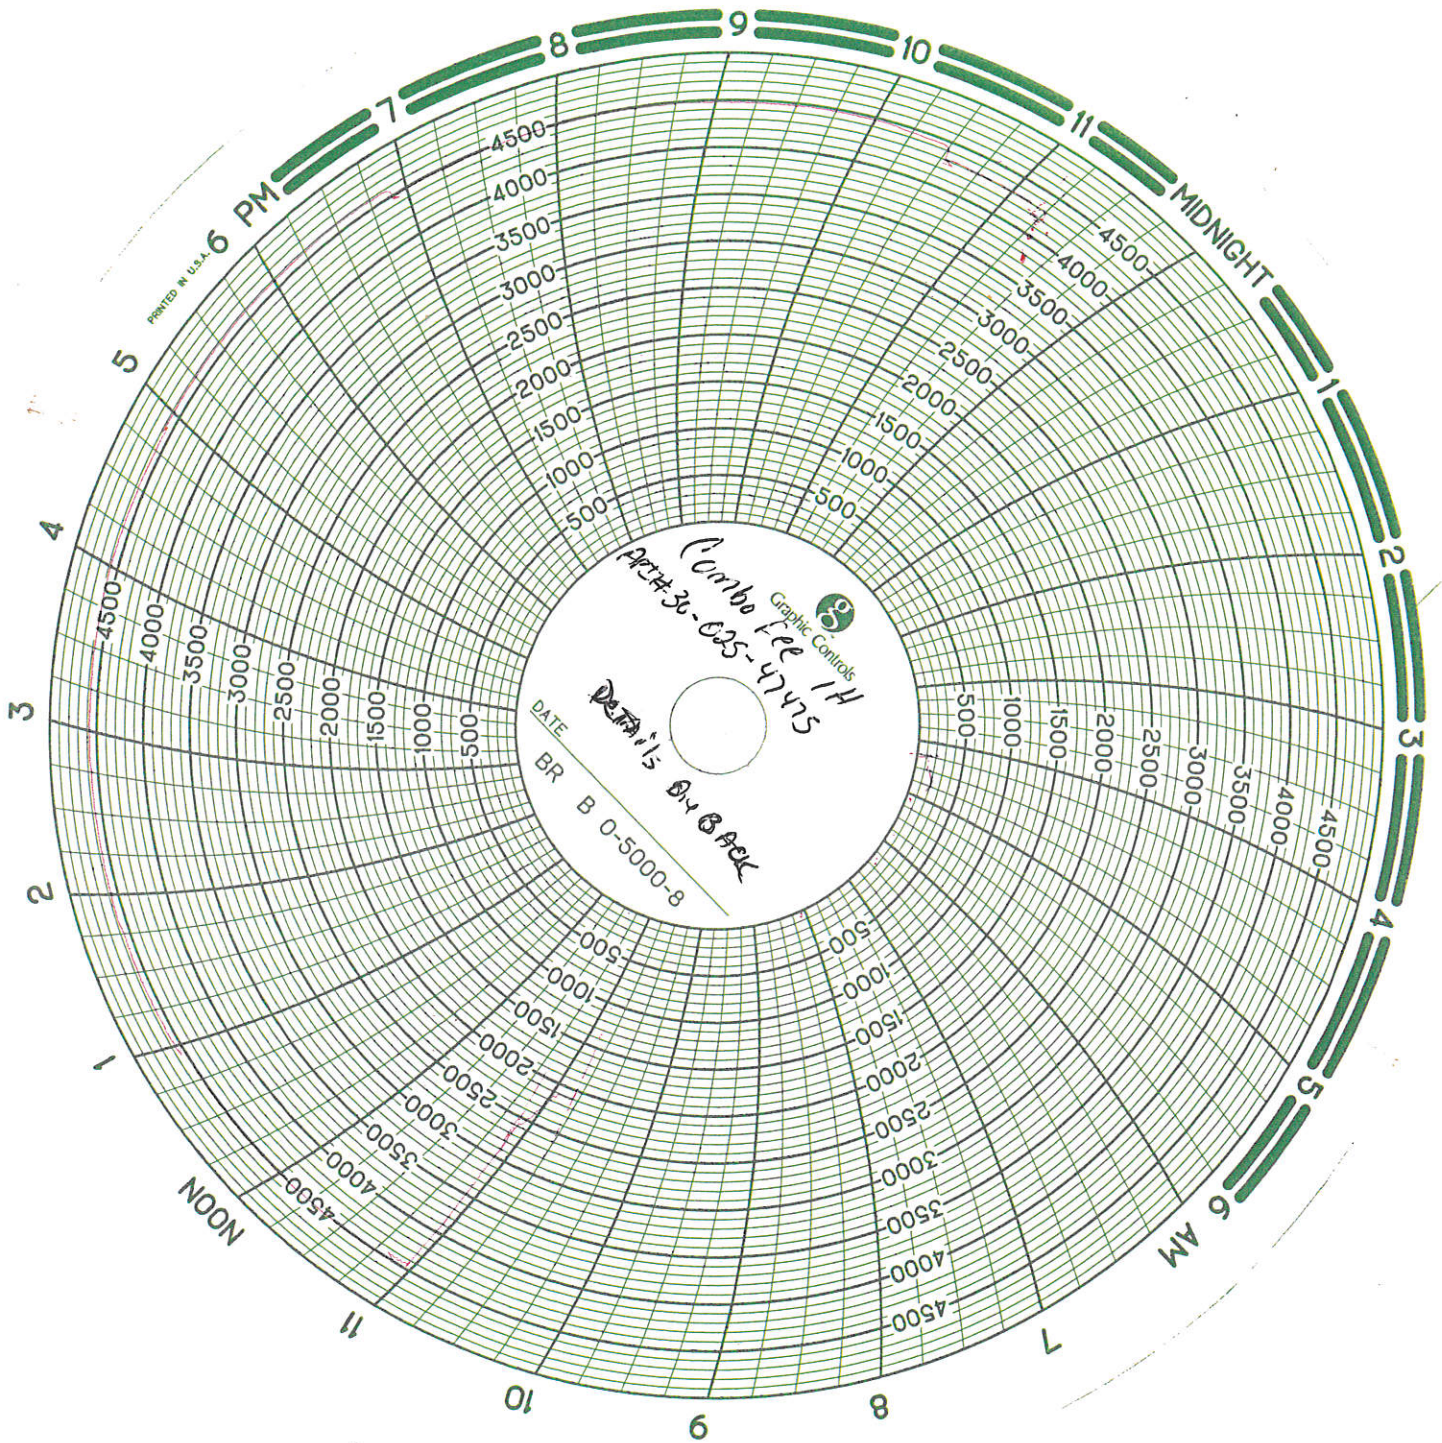

30min test

30-025-47475

API# Valve & meta Inc

APPLICANT BA342

Serial B2342

Calibration by Susan Harris

Reviewed by

Witness by

Heart Fields

DATE 12/11/2020

American Valve & Meter, Inc.

1113 W. BROADWAY

P.O. BOX 166 HOBBS, NM 88240

T0: Rental

DATE:12/11/20

This is to certify that:

I, Justin Harris, Technician for American Valve & Meter Inc. has checked the calibration of the following instrument.

08" Pressure Recorder


Ser#B2342

at these points

Pressure #			Temperature *or Pressure #		
Test	Found	Left	Test	Found	Left
- 0	-	- 0	-	-	-
- 2500	-	- 2500	-	-	-
- 5000	-	-5000	-	-	-
- 4000	-	-4000	-	-	-
- 1000	-	- 1000	-	-	-
- 0	-	- 0			

Remarks: _____

Signature: _____

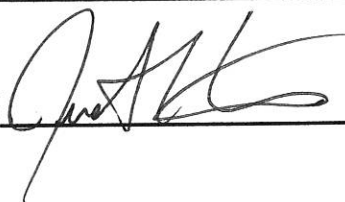

1220 S. St Francis Dr., Santa Fe, NM 87505
Phone:(505) 476-3470 Fax:(505) 476-3462

Action 12752

OCD Reviewer	Condition
pkautz	None