


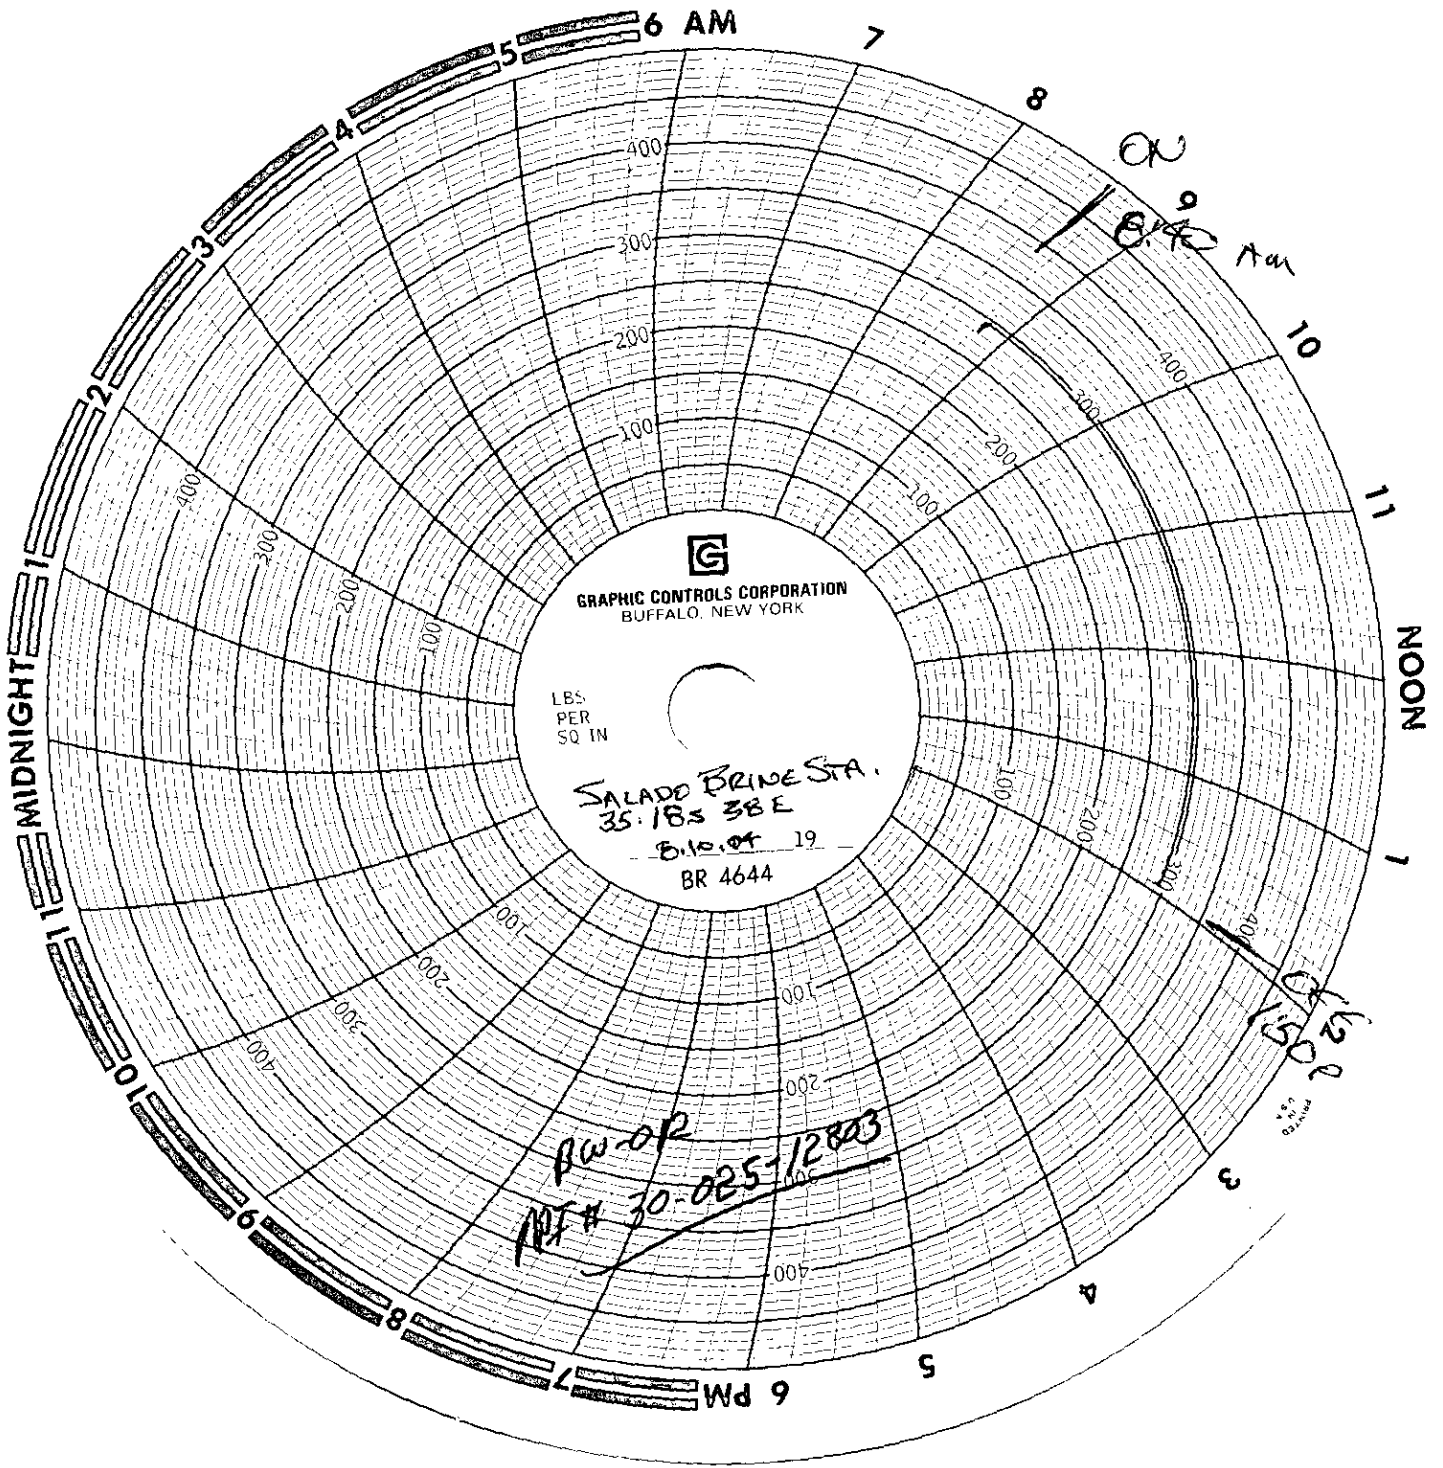

8-10-04 ON 8:30
OFF 1:30


Dennis Shearn

~~John P. Shearn~~

William G.

SALINE BRINE

35 18S 37E

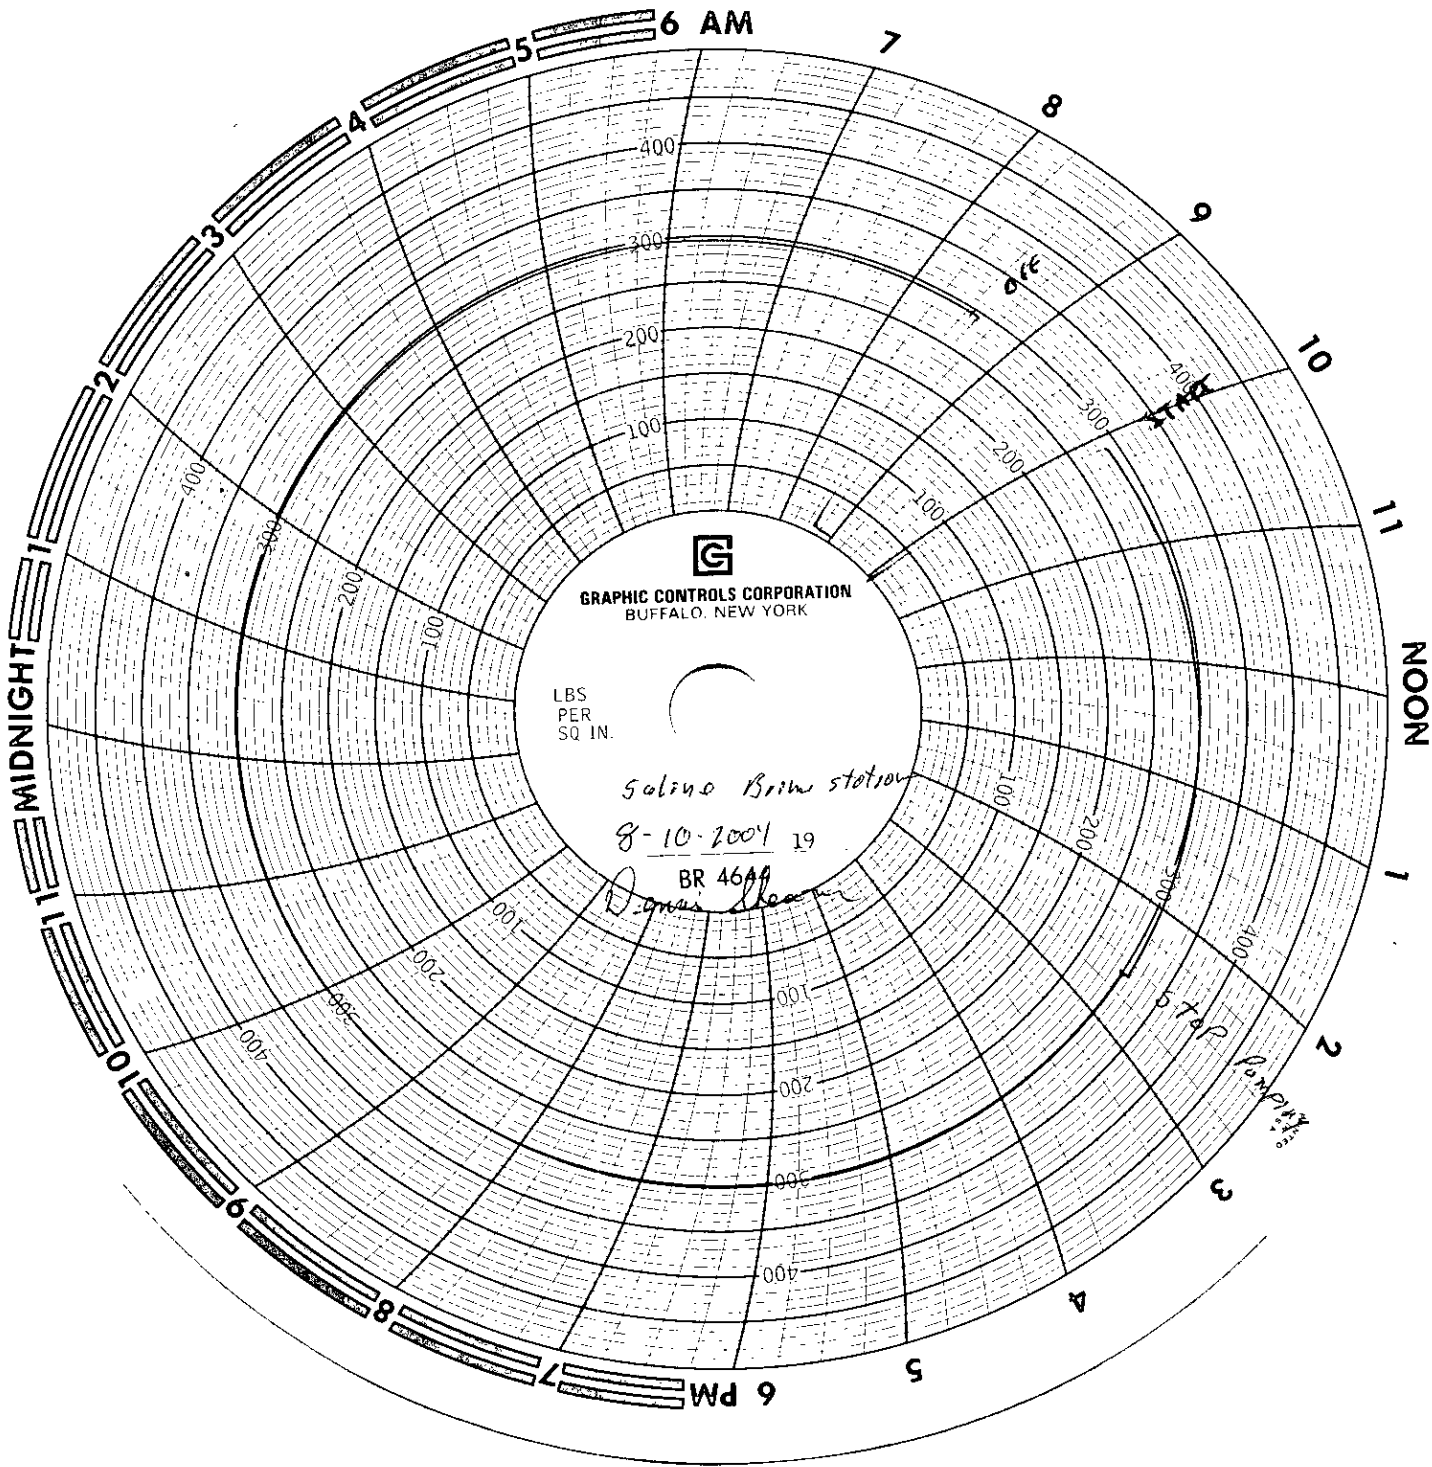

American Valve & Meter, Inc.

113 W. Broadway
P.O. Box 155
Hobbs, NM 88240

To: Plains

Date: 4/6/04

This is to Certify that:

I, David L. Hall, Technician for American Valve & Meter, Inc.,

has checked the calibration of the following instrument

2" Pressure recorder Serial Number 19530

at these points:

Pressure 10-500

Temperature _____

Test	Found	Left	Test	Found	Left
<u>0</u>	<u>rechecked</u>	<u>0</u>	_____	_____	_____
<u>250</u>	_____	<u>250</u>	_____	_____	_____
<u>500</u>	_____	<u>500</u>	_____	_____	_____
<u>350</u>	_____	<u>350</u>	_____	_____	_____
<u>150</u>	_____	<u>150</u>	_____	_____	_____
<u>0</u>	_____	<u>0</u>	_____	_____	_____

Remarks: _____

Signature

David L. Hall

8-10-09



PLAINS
MARKETING, L.P.

Plains Marketing GP Inc.
General Partner

Dennis Shearer
Truck Supervisor

3514 Lovington Hwy.
Hobbs, NM 88240

Phone: 505-392-6559

Fax: 505-392-6988

Mobile: 505-369-6642

Res: 505-397-7538

Toll Free: 800-238-8629

dlshearer@paalp.com
