


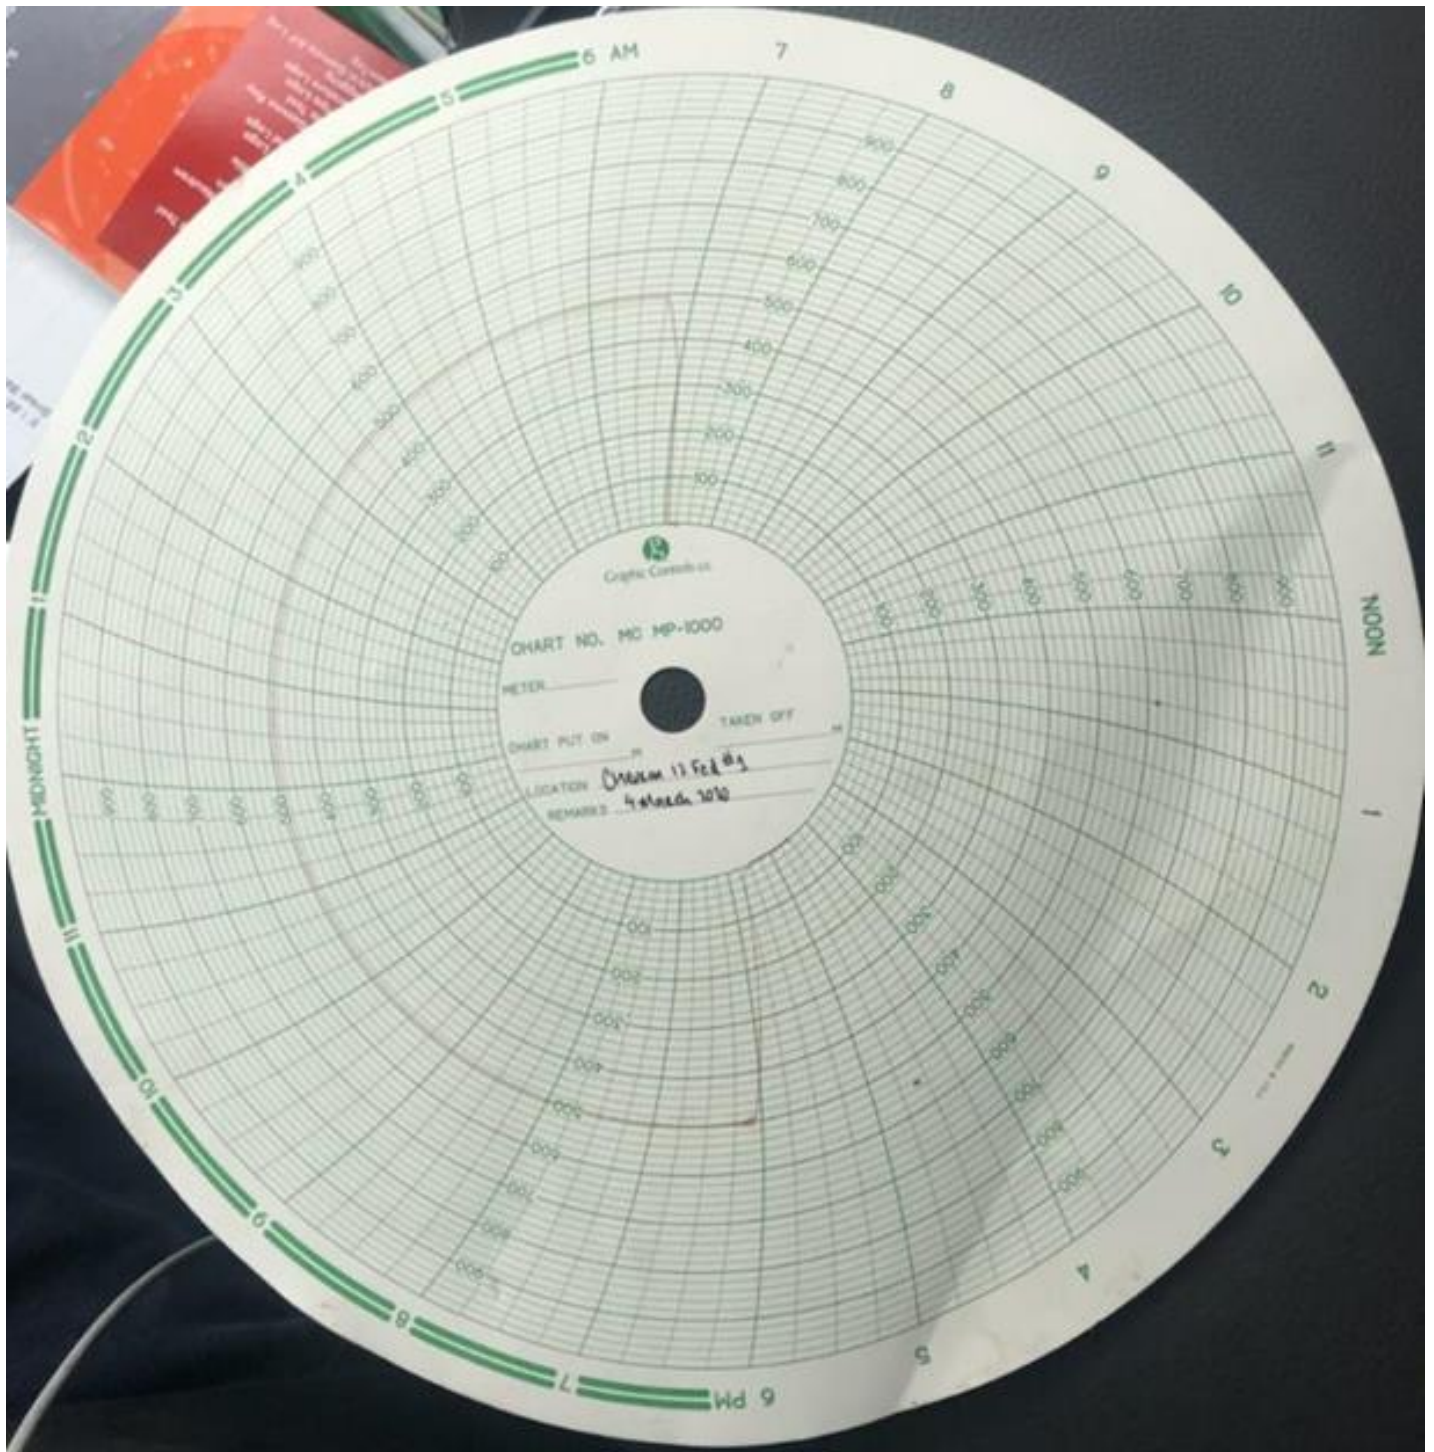

124 Credit Dr.
Scott, LA 70583
Phone (337)237-7675
Fax (337)237-7676

Atchafalaya

MEASUREMENT, INC.

Houma, LA 70360
Phone (985)851-6077

Calibration Certificate

Company Name: 2 Brothers Services

Recorder Type: Barton

Recorder Serial#: 263-6193

Recorder Pressure Range: 0-1000# Accuracy +/-: 0.2% PSIG

Temperature Range: 0-150 Deg F. Accuracy +/-: 2% Deg F

Increasing Pressure			Decreasing Pressure		
Applied Pressure	Indicated Pressure	Error%	Applied Pressure	Indicated Pressure	Error%
0.0#	0.0#	0	800#	800#	0
100#	100#	0	600#	600#	0
300#	300#	0	400#	400#	0
500#	500#	0	200#	200#	0
700#	700#	0	0.0#	0.0#	0

Certified Calibration Instrument Used

Gauge: Crystal

Deadweight: _____

Remarks: _____

Calibration Date: 2/11/2020

Technician: _____

Karl Haeny