


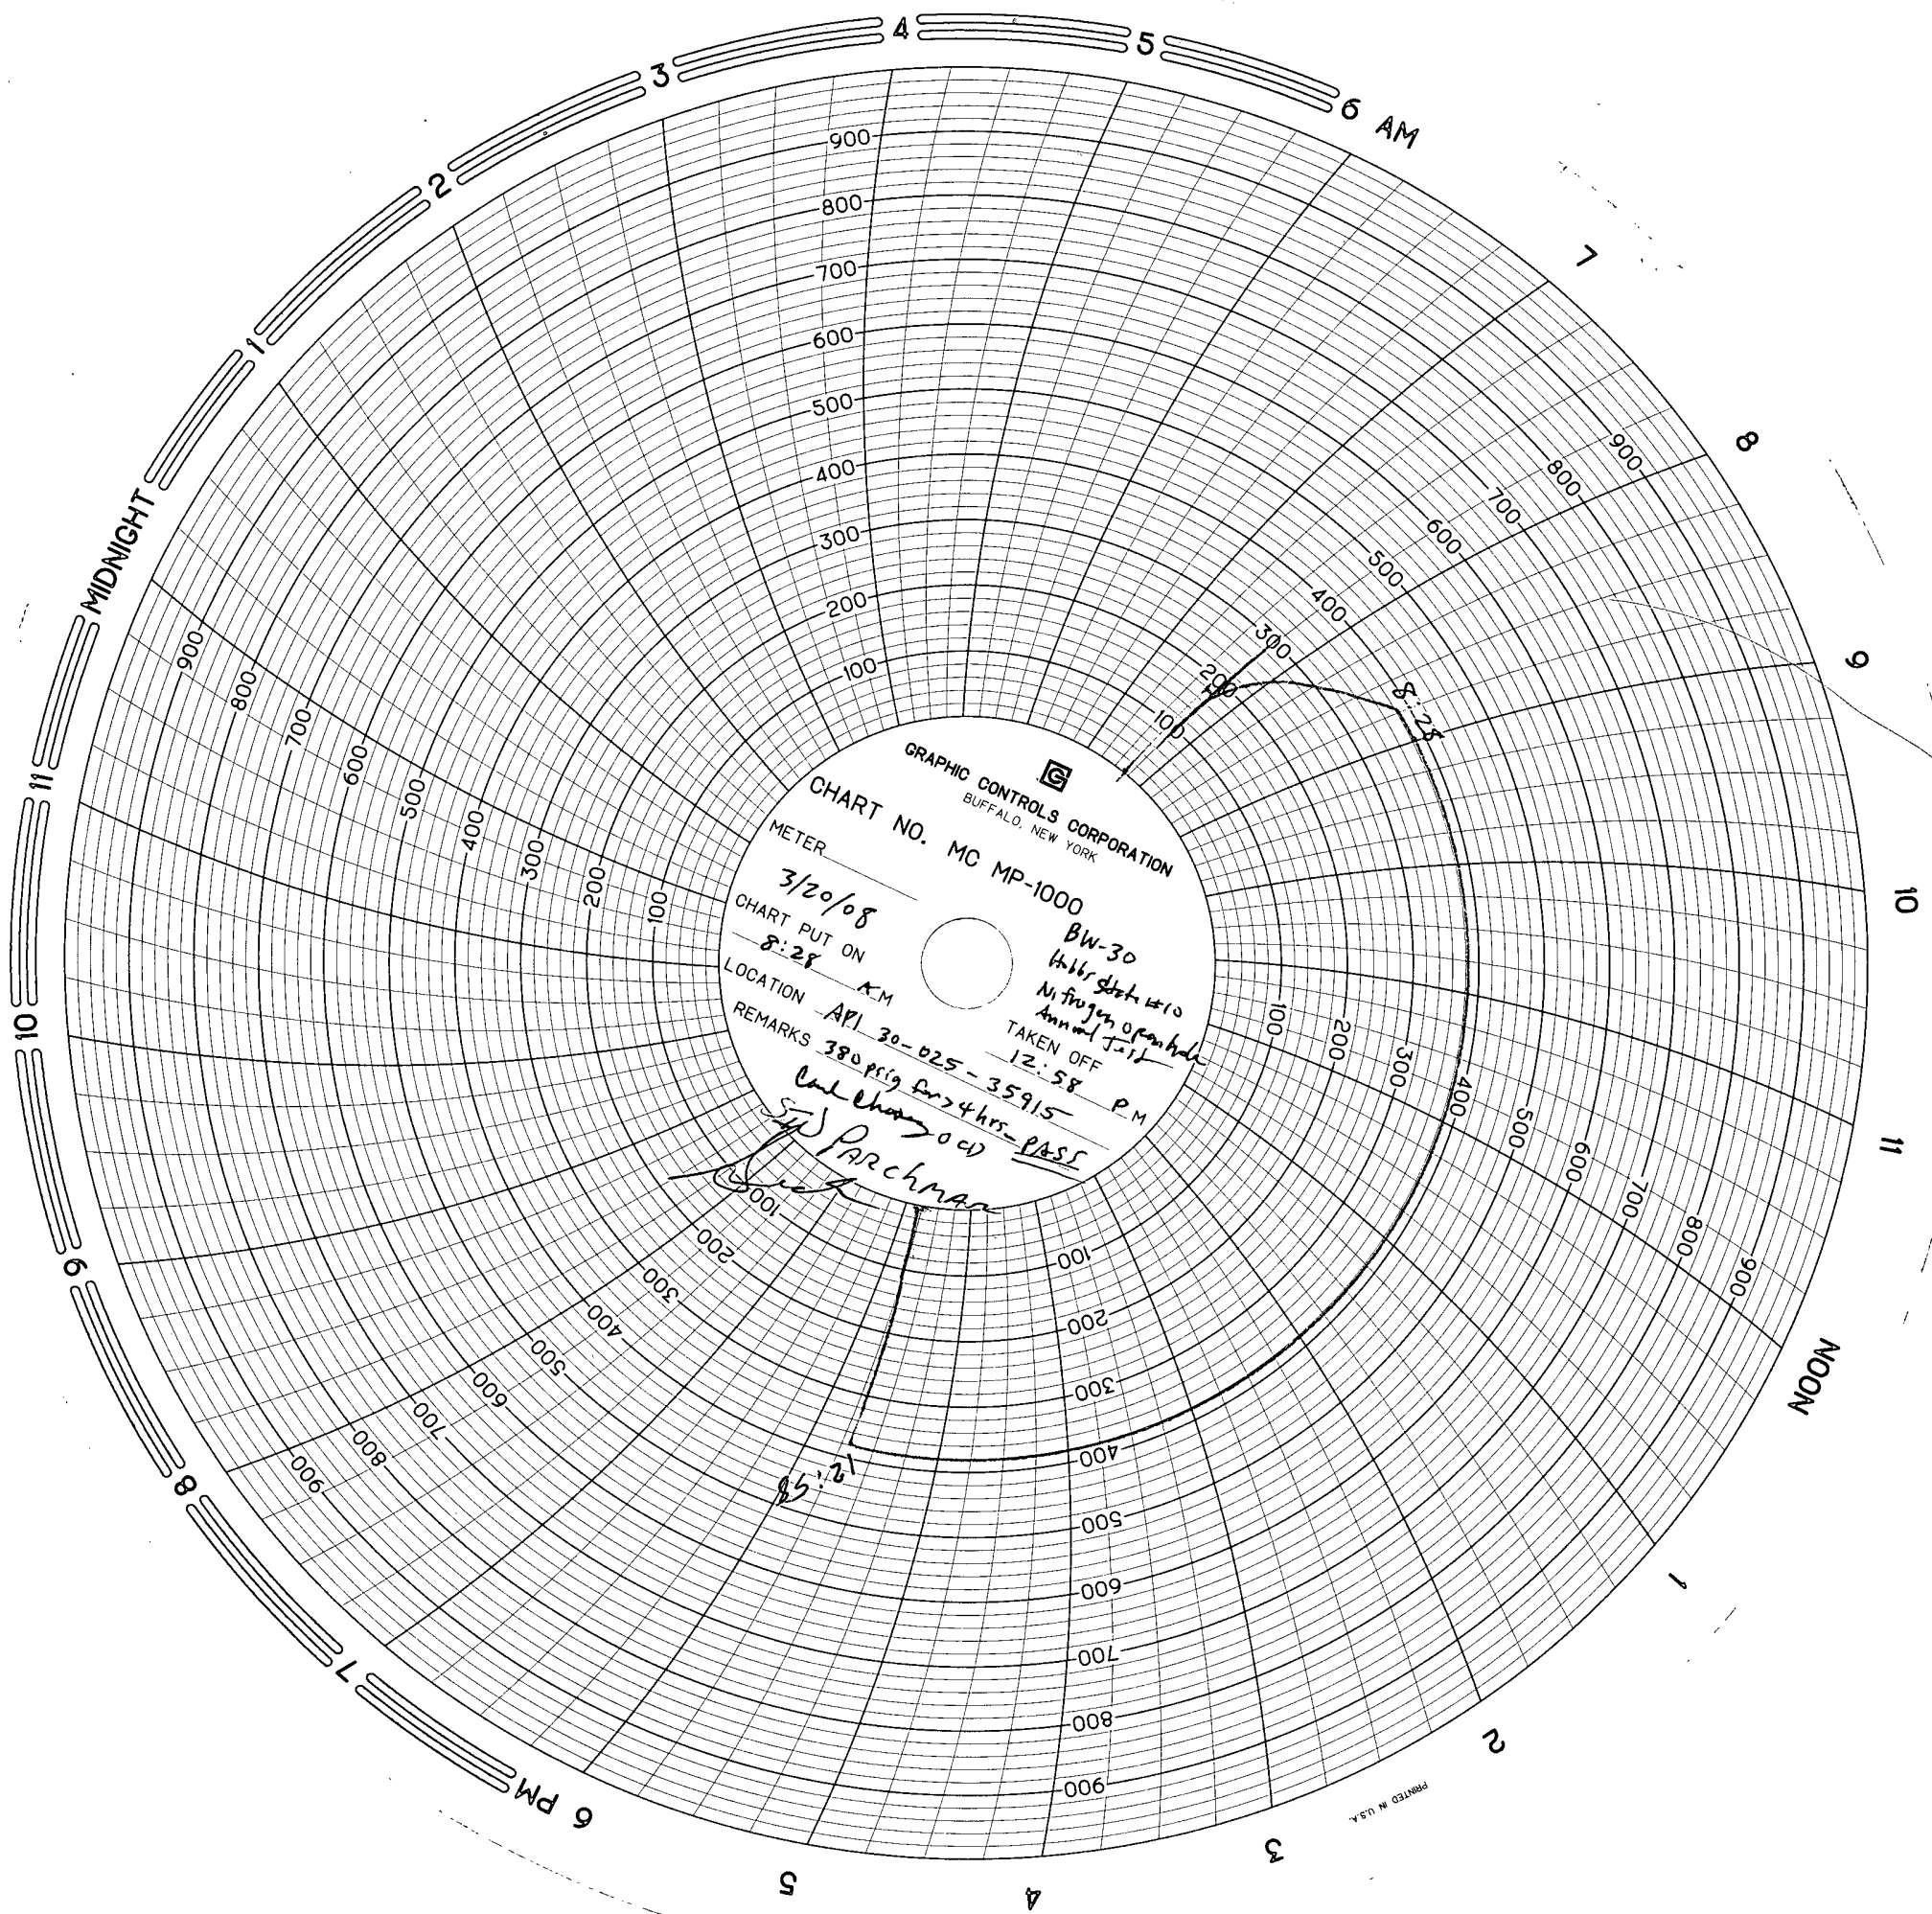

GRAPHIC CONTROLS CORPORATION
BUFFALO, NEW YORK

CHART NO. MC MP-1000

METER 3/20/68

CHART PUT ON 8:28

LOCATION K.M

REMARKS 380 ftig for 4 hrs - PASS

TAKEN OFF 12:58 P.M.

S. J. PARCHMAN

PRINTED IN U.S.A.

BW-30

3/20/08

American Valve & Meter, Inc.

1113 W. BROADWAY

P.O. BOX 166

HOBBS, NM 88240

TO: TRMDATE: 3/10/08

This is to certify that:

I, Bud Collins, Technician for American Valve & Meter,
Inc., has checked the calibration of the following instrument.

12" pressure recorder Serial No: 19331

at these points.

Pressure 0 - 1000 PSI

Temperature _____

<u>Test</u>	<u>Found</u>	<u>Left</u>	<u>Test</u>	<u>Found</u>	<u>Left</u>
<u>0</u>	—	<u>0</u>	—	—	—
<u>500</u>	—	<u>500</u>	—	—	—
<u>1000</u>	—	<u>1000</u>	—	—	—
<u>700</u>	—	<u>700</u>	—	—	—
<u>200</u>	—	<u>200</u>	—	—	—
<u>0</u>	—	<u>0</u>	—	—	—

Remarks: _____

Signature Bud Collins