




500 → 495 / 30 min

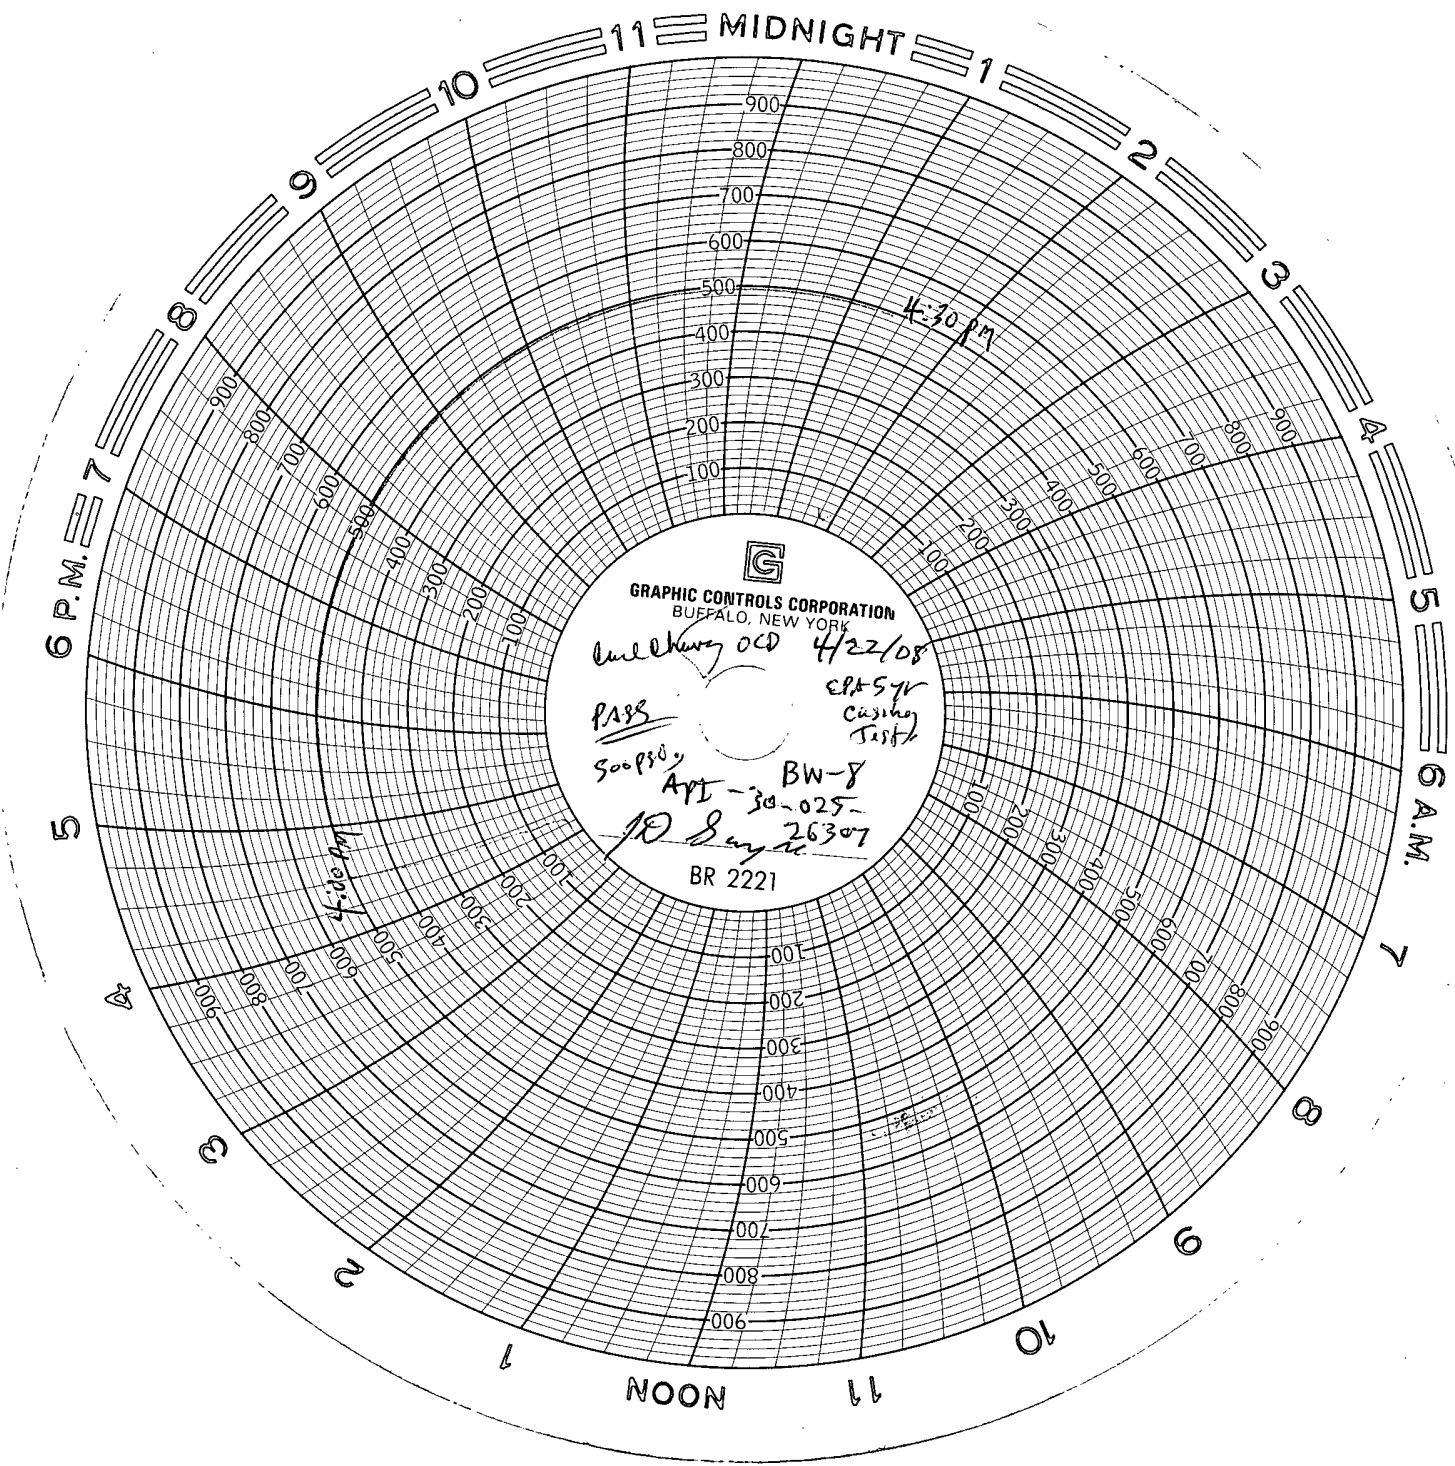

BW-8 4/22/08

4:00 PM

American Valve & Meter, Inc.

1113 W. BROADWAY

P.O. BOX 166

HOBBS, NM 88240

TO: ZIADATE: 9-20-07

This is to certify that:

I, Bud Collins, Technician for American Valve & Meter,
Inc., has checked the calibration of the following instrument.

8" pressure recorder Serial No: 501

at these points.

Pressure 0-1000

Temperature _____

<u>Test</u>	<u>Found</u>	<u>Left</u>	<u>Test</u>	<u>Found</u>	<u>Left</u>
<u>0</u>	<u>—</u>	<u>0</u>	<u>—</u>	<u>—</u>	<u>—</u>
<u>500</u>	<u>—</u>	<u>500</u>	<u>—</u>	<u>—</u>	<u>—</u>
<u>1000</u>	<u>—</u>	<u>1000</u>	<u>—</u>	<u>—</u>	<u>—</u>
<u>700</u>	<u>—</u>	<u>700</u>	<u>—</u>	<u>—</u>	<u>—</u>
<u>200</u>	<u>—</u>	<u>200</u>	<u>—</u>	<u>—</u>	<u>—</u>
<u>0</u>	<u>—</u>	<u>0</u>	<u>—</u>	<u>—</u>	<u>—</u>

Remarks: _____

Signature Bud Collins