


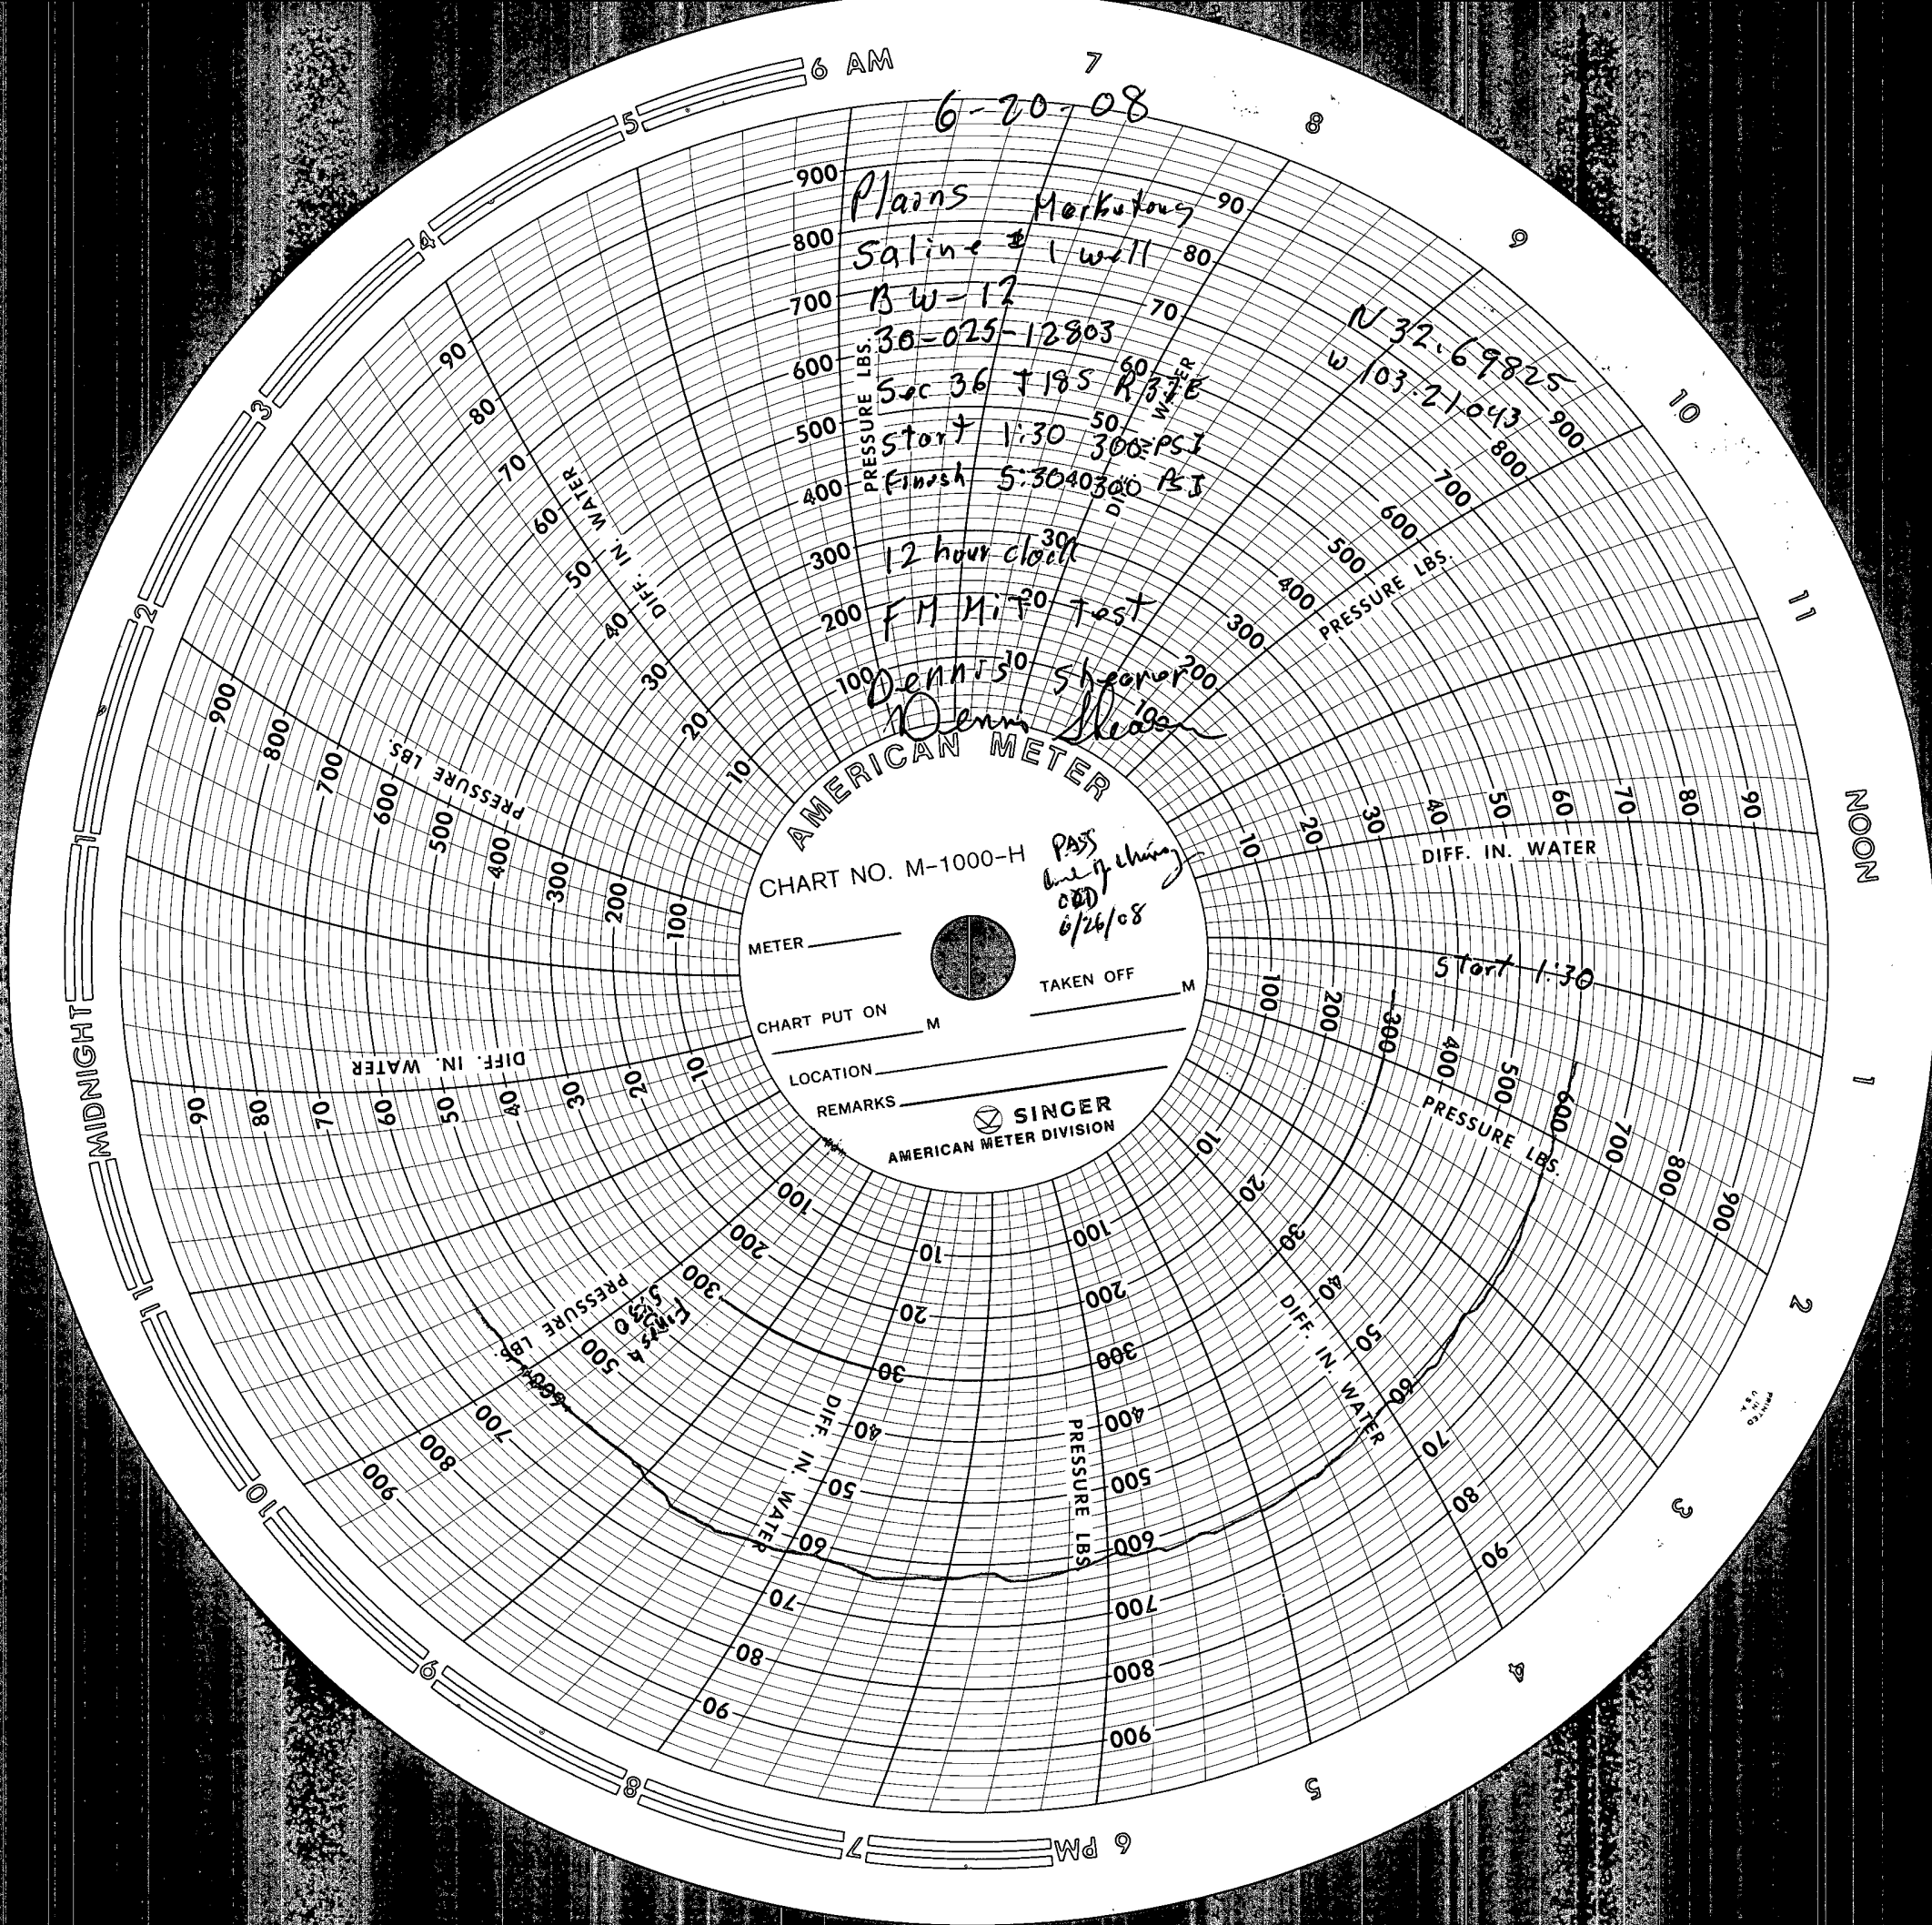

American Valve & Meter, Inc.

1113 W. BROADWAY

P.O. BOX 166

HOBBS, NM 88240

TO: Plains

DATE: 3-10-08

This is to certify that:

I, Bud Collins, Technician for American Valve & Meter, Inc., has checked the calibration of the following instrument.

22" Press./Temp recorder Serial No: 240015

at these points.

Pressure 0-1000

Temperature 0-150°

<u>Test</u>	<u>Found</u>	<u>Left</u>	<u>Test</u>	<u>Found</u>	<u>Left</u>
<u>0</u>	<u>—</u>	<u>0</u>	<u>32</u>	<u>—</u>	<u>32</u>
<u>500</u>	<u>—</u>	<u>500</u>	<u>71</u>	<u>—</u>	<u>71</u>
<u>1000</u>	<u>—</u>	<u>1000</u>	<u>148</u>	<u>—</u>	<u>148</u>
<u>700</u>	<u>—</u>	<u>740</u>	<u>—</u>	<u>—</u>	<u>—</u>
<u>200</u>	<u>—</u>	<u>200</u>	<u>—</u>	<u>—</u>	<u>—</u>
<u>0</u>	<u>—</u>	<u>0</u>	<u>—</u>	<u>—</u>	<u>—</u>

Remarks: _____

Signature Bud Collins

RECEIVED

2008 JUN 26 PM 3:45